



CERTIFICATE OF ANALYSIS

Product: Human LOXL2 ELISA Kit

Catalog No: OKEH02393

Lot No: KF0668

Expiration Date: 2021.11

Performance Characteristics:

Intra-Assay CV	< 5.4%	Passed
Inter-Assay CV	< 8.6%	Passed
Limit of Detection (LOD)		< 9.4 pg/mL
Assay Range		78 – 5,000 pg/mL

Standard Dilution:


Prepare the standards immediately before use. For each experiment, add 2 mL of Sample Diluent to the 40,000 pg Lyophilized LOXL2 Standard. Mix gently until dissolved. Leave the vial at ambient temperature for 15 minutes.

Prepare a 5,000 pg/mL Standard by adding 250 µL of 20,000 pg/mL Standard to 750 µL of Sample Diluent in Tube #1. Mix gently and thoroughly.

Standard Number (Tube)	Standard to Dilute	Volume Standard to Dilute (µL)	Volume Sample Diluent (µL)	Total Volume (µL)	Final Concentration (pg/mL)
Standard	40,000 pg/mL LOXL2 Standard	NA	2,000	2,000	20,000 pg/mL
1	20,000 pg/mL	250	750	1,000	5,000 pg/mL
2	5,000 pg/mL	300	300	600	2,500 pg/mL
3	2,500 pg/mL	300	300	600	1,250 pg/mL
4	1,250 pg/mL	300	300	600	625 pg/mL
5	625 pg/mL	300	300	600	312 pg/mL
6	312 pg/mL	300	300	600	156 pg/mL
7	156 pg/mL	300	300	600	78 pg/mL
8	N/A	0	300	300	0.0 (Blank)

Sample Standard Curve and Calculations ONLY. Do not use below report for result calculations. A standard curve should be generated each time the test is performed

Standard Curve Graph

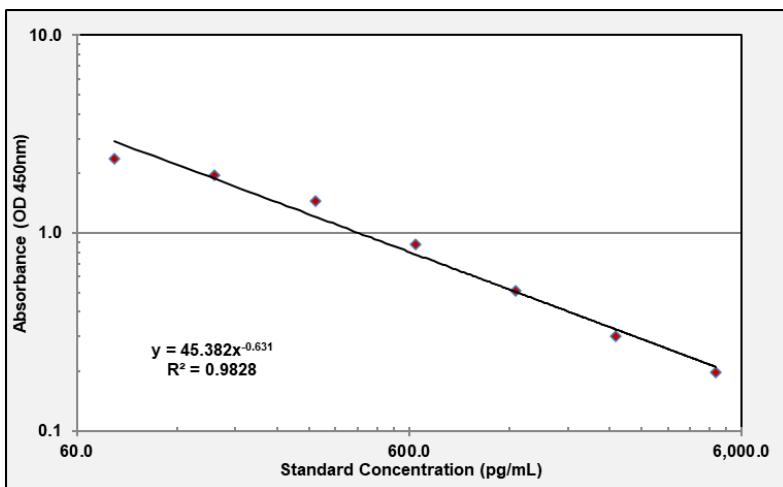

Standard pg/mL	Absorbance (OD 450nm)
5,000	0.198
2,500	0.302
1,250	0.509
625	0.876
313	1.443
156	1.955
78	2.388