



## CERTIFICATE OF ANALYSIS

**Product:** Human SDCBP ELISA Kit

**Catalog No:** OKEH02415

**Lot No:** KG0090

**Expiration Date:** 2022.08

**Performance Characteristics:**

Intra-Assay CV	< 5.4%	Passed
Inter-Assay CV	< 8.1%	Passed
Limit of Detection (LOD)		< 0.012 ng/mL
Assay Range		0.312 – 20 ng/mL

**Standard Dilution:**


Prepare the standards immediately before use. For each experiment, add 2 mL of Sample Diluent to the 80 ng Lyophilized SDCBP Standard. Mix gently until dissolved. Leave the vial at ambient temperature for 15 minutes.

Prepare a 20 ng/mL Standard by adding 500 µL of 40 ng/mL Standard to 500 µL of Sample Diluent in Tube #1. Mix gently and thoroughly.

Standard Number (Tube)	Standard to Dilute	Volume Standard to Dilute (µL)	Volume Sample Diluent (µL)	Total Volume (µL)	Final Concentration (ng/mL)
Standard	80 ng SDCBP Standard	NA	2,000	2,000	40 ng/mL
1	40 ng/mL	500	500	1,000	20 ng/mL
2	20 ng/mL	300	300	600	10 ng/mL
3	10 ng/mL	300	300	600	5.0 ng/mL
4	5.0 ng/mL	300	300	600	2.5 ng/mL
5	2.5 ng/mL	300	300	600	1.25 ng/mL
6	1.25 ng/mL	300	300	600	0.625 ng/mL
7	0.625 ng/mL	300	300	600	0.312 ng/mL
8	N/A	0	300	300	0.0 (Blank)

Sample Standard Curve and Calculations ONLY. Do not use below report for result calculations. A standard curve should be generated each time the test is performed

### Standard Curve Graph

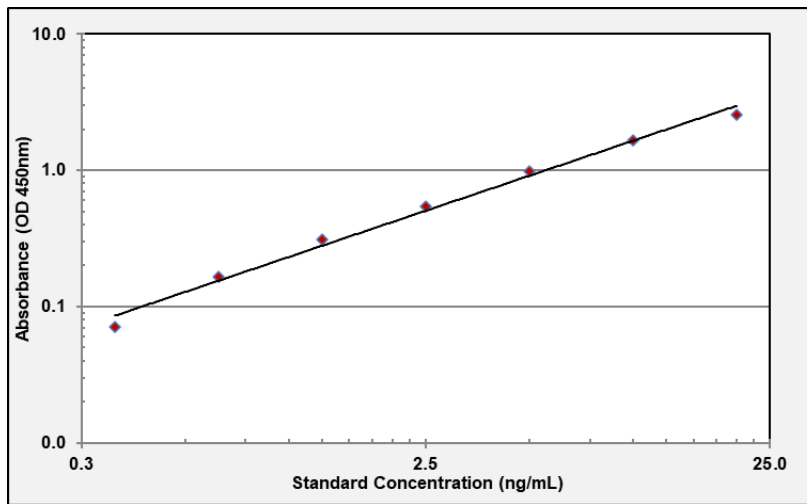

Standard ng/mL	Absorbance (OD 450nm)
20	2.579
10	1.668
5.0	0.984
2.5	0.542
1.25	0.313
0.625	0.164
0.313	0.071