

CERTIFICATE OF ANALYSIS

Product: SERPINA3 ELISA Kit (Human)
SKU: OKEH02895
Lot: KH0781
Expiration Date: 2024.05

Performance Characteristics:

Intra-Assay CV	$\leq 4.3\%$	Passed
Inter-Assay CV	$\leq 5.5\%$	Passed
Limit of Detection (LOD)		$\leq 0.78 \text{ umol/L}$
Assay Range		1.56 - 100 umol/L


Standard Preparation:

Prepare the standards immediately before use. For each experiment, add 1 mL of Sample Diluent to the 100 umol Lyophilized SERPINA3 standard. Mix gently until dissolved. Leave the vial at ambient temperature for 15 minutes.

Prepare a set of diluted standards as indicated in the chart below:

Standard Number (Tube)	Standard To Dilute	Volume Standard To Dilute (uL)	Volume Sample Diluent Buffer (uL)	Total Volume (uL)	Final Concentration (umol/L)
1	Reconstitute SERPINA3 Standard	N/A	N/A	1,000	100
2	100	300	300	600	50

Standard Number (Tube)	Standard To Dilute	Volume Standard To Dilute (uL)	Volume Sample Diluent Buffer (uL)	Total Volume (uL)	Final Concentration (umol/L)
3	50	300	300	600	25
4	25	300	300	600	12.5
5	12.5	300	300	600	6.25
6	6.25	300	300	600	3.12
7	3.12	300	300	600	1.56
8	N/A	0	300	300	0.0 (Blank)

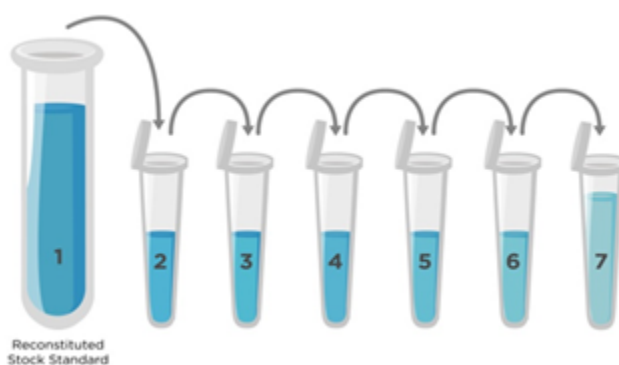

Typical Expected Data

Standard Curve and Calculations ONLY. Do not use below report for result calculations. A standard curve should be generated each time the test is performed.

Standard Number	Concentration (umol/L)	Background Adjusted OD Value
1	100	2.156
2	50	1.168
3	25	0.645
4	12.5	0.34
5	6.25	0.164
6	3.12	0.087

Standard Number	Concentration (umol/L)	Background Adjusted OD Value
7	1.56	0.052

Standard Curve Graph

