

**Human FGF-basic ELISA KIT**

Catalog Number  
OKAA00030\_96W

Size  
96 Tests



---

**Human FGF-basic ELISA KIT**

**For the quantitative determination of human Fibroblast Growth Factor-basic (FGF-b, FGF-2) concentrations in cell culture supernates, serum, and plasma. This package insert must be read in its entirety before using this product. If you have questions or experience problems with this product, please contact our Technical Support staff. Our scientists commit themselves to providing rapid and effective help.**

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

**AVIVA SYSTEMS BIOLOGY**

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com

## INTRODUCTION

FGF basic, also called FGF-2 (fibroblast growth factor-2) or HBGF-2 (heparin-binding growth factor-2), is the most intensively studied of the 22 mitogenic proteins of the FGF family (1-7). Family members share 35 - 60% amino acid (aa) identity, but only FGF acidic and basic lack signal peptides and are secreted by an alternate pathway.

The 18 kDa FGF basic isoform can be found in both the cytoplasm and the nucleus and is also the form that is secreted (8-10). Storage pools within the cell or on cell surface heparan sulfate proteoglycans (HSPG) are likely (2). Transcription from alternate start sites produces 21-23 kDa forms found only in the nucleus (8, 9). High and low molecular weight human FGF basic isoforms target the expression of different genes (9, 10). The 18 kDa human FGF basic sequence shares 97% and 99% aa identity with mouse/rat and bovine/ovine FGF basic, respectively (6, 7). Expression of FGF basic is nearly ubiquitous. However, disruption of the mouse FGF basic gene gives relatively mild cardiovascular, skeletal, and neuronal phenotypes, suggesting compensation by other FGF family members (11-15). Transgenic over-expression of FGF basic mainly influences development and mineralization of bone (4, 16, 17).

Four FGF tyrosine kinase receptors (FGF R) and their splice variants show differential binding of FGFs (1). FGF basic preferentially binds FGF R1c and 2c, for which it has picomolar affinity (1, 2). FGF basic also has a number of other binding partners that fine-tune FGF basic activities, according to their locations and quantities. FGF basic modulates such normal processes as angiogenesis, wound healing, tissue repair, learning and memory, and embryonic development and differentiation of heart, bone and brain (2 - 4). It is upregulated in response to inflammation via mediators such as TNF- $\alpha$ , IL-1 $\beta$ , IL-2, PDGF, and nitric oxide (2). Many human tumors express FGF basic, which may correlate with tumor vascularity (2, 5).

## PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. A monoclonal antibody specific for FGF-basic has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any FGF-basic present is bound by the immobilized antibody. Following incubation unbound samples are removed during a wash step,


FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

### AVIVA SYSTEMS BIOLOGY

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com

and then a detection antibody specific for FGF-basic is added to the wells and binds to the combination of capture antibody- FGF-basic in sample. Following a wash to remove any unbound combination, and enzyme conjugate is added to the wells. Following incubation and wash steps a substrate is added. A coloured product is formed in proportion to the amount of FGF-basic present in the sample. The reaction is terminated by addition of acid and absorbance is measured at 450nm. A standard curve is prepared from seven FGF-basic standard dilutions and FGF-basic sample concentration determined.

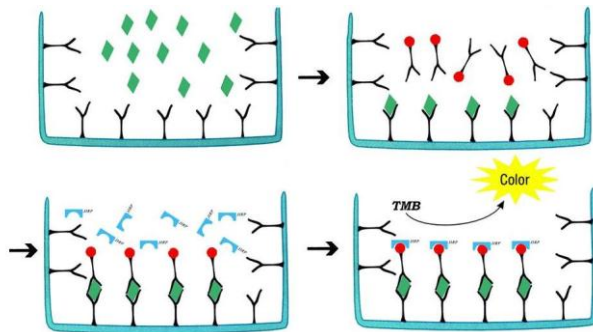

**Figure 1: Schematic diagram of the assay**

## REAGENTS

1. Aluminum pouches with a Microwell Plate coated with antibody to human FGF-basic (8×12)
2. 2 vials human FGF-basic Standard lyophilized, 500 pg/ml upon reconstitution
3. 2 vials concentrated Biotin-Conjugate anti-human FGF-basic antibody
4. 2 vials Streptavidin-HRP solution,
5. 1 bottle Standard /sample Diluent
6. 1 bottle Biotin-Conjugate antibody Diluent
7. 1 bottle Streptavidin-HRP Diluent
8. 1 bottle Wash Buffer Concentrate 20x (PBS with 1% Tween-20)
9. 1 vial Substrate Solution
10. 1 vial Stop Solution
11. 4 pieces Adhesive Films

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

### AVIVA SYSTEMS BIOLOGY

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
 www.avivasysbio.com | Email: info@avivasysbio.com

12. package insert

**NOTE:** [96 Tests]

## STORAGE

Table 1: Storage of the kit

<b>Unopened Kit</b>	Store at 2 - 8° C. Do not use past kit expiration date.	
<b>Opened/ Reconstituted Reagents</b>	Standard /sample Diluent	May be stored for up to 1 month at 2 - 8° C.**
	Concentrated Biotin-Conjugate	
	Streptavidin-HRP solution	
	Biotin-Conjugate antibody Diluent	
	Streptavidin-HRP Diluent	
	Wash Buffer Concentrate 20x	
	Substrate Solution	
	Stop Solution	
	Standard	Aliquot and store for up to 1 month at ≤20°C. Avoid repeated freeze-thaw cycles. Diluted standard shall not be reused.
	Microplate Wells	Return unused wells to the foil pouch containing the desiccant pack, reseal along entire edge of zip-seal. May be stored for up to 1 month at 2 - 8° C.**

\*\*Provided this is within the expiration date of the kit.

### THE REQUIRED ITEMS (not provided, but can help to buy):

1. Microplate reader (450nm).
2. Micro-pipette and tips: 0.5-10, 2-20, 20-200, 200-1000ul.
3. 37 ° C incubator, double-distilled water or deionized water, coordinate paper, graduated cylinder.

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

#### AVIVA SYSTEMS BIOLOGY

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com

## PRECAUTIONS FOR USE

1. Store kit reagents between 2° C and 8° C. After use all reagents should be immediately returned to cold storage (2° C to 8° C).
2. Please perform simple centrifugation to collect the liquid before use.
3. To avoid cross contamination, please use disposable pipette tips.
4. The Stop Solution suggested for use with this kit is an acid solution. Wear eye, hand, face, and clothing protection when using this material. Avoid contact of skin or mucous membranes with kit reagents or specimens. In the case of contact with skin or eyes wash immediately with water.
5. Use clean, dedicated reagent trays for dispensing the washing liquid, conjugate and substrate reagent. Mix all reagents and samples well before use.
6. After washing microtiter plate should be fully pat dried. Do not use absorbent paper directly into the enzyme reaction wells.
7. Do not mix or substitute reagents with those from other lots or other sources. Do not use kit reagents beyond expiration date on label.
8. Each sample, standard, blank and optional control samples should be assayed in duplicate or triplicate.
9. Adequate mixing is very important for good result. Use a mini-vortexer at the lowest frequency or Shake by hand at 10min interval when there is no vortexer.
10. Avoid microtiter plates drying during the operation.
11. Dilute samples at the appropriate multiple, and make the sample values fall within the standard curve. If samples generate values higher than the highest standard, dilute the samples and repeat the assay.
12. Any variation in standard diluent, operator, pipetting technique, washing technique, incubation time and temperature, and kit age can cause variation in binding.
13. This method can effectively eliminate the interference of the soluble receptors, binding proteins and other factors in biological samples.

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

### **AVIVA SYSTEMS BIOLOGY**

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com

## **SAMPLE COLLECTION AND STORAGE**

1. **Cell Culture Supernates** - Remove particulates by centrifugation.
2. **Serum** - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at approximately 1000 x g. Remove serum, avoid hemolysis and high blood lipid samples.
3. **Plasma** - Recommended EDTA as an anticoagulant in plasma. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection.
4. Assay immediately or aliquot and store samples at -20° C. Avoid repeated freeze-thaw cycles.
5. Dilute samples at the appropriate multiple (recommended to do pre-test to determine the dilution factor).

## **REAGENT PREPARATION**

1. Bring all reagents to room temperature before use.
2. **Wash Buffer** - Dilute 10mL of Wash Buffer Concentrate into deionized or distilled water to prepare 200mL of Wash Buffer. If crystals have formed in the concentrate Wash Buffer, warm to room temperature and mix gently until the crystals have completely dissolved.
3. **Standard** - Reconstitute the Standard with 1.0mL of Standard /sample Diluent. This reconstitution produces a stock solution of 500 pg /mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions.

Pipette 500µL of Standard/sample Diluent into the 250 pg/mL tube and the remaining tubes. Use the stock solution to produce a 2-fold dilution series (below). Mix each tube thoroughly and change pipette tips between each transfer. The 500 pg/mL standard serves as the high standard. The Standard/ sample Diluent serves as the zero standard (0 pg/mL).

**If you do not run out of re-melting standard, store it at -20° C. Diluted standard shall not be reused.**

4. Working solution of Biotin-Conjugate anti-human FGF-basic antibody: Make a 1:100 dilution of the concentrated Biotin-Conjugate solution with the Biotin-Conjugate antibody Diluent in a clean plastic tube.

**The working solution should be used within one day after dilution.**

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.


---

### **AVIVA SYSTEMS BIOLOGY**

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com

5. Working solution of Streptavidin-HRP: Make a 1:100 dilution of the concentrated Streptavidin-HRP solution with the Streptavidin-HRP Diluent in a clean plastic tube.

**The working solution should be used within one day after dilution.**

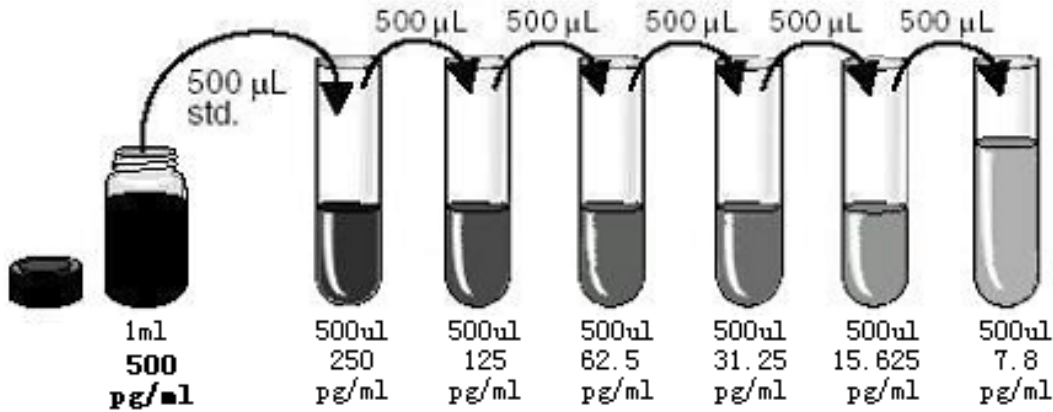

**Figure 2: Preparation of FGF-basic standard dilutions**

## GENERAL ELISA PROTOCOL

1. Prepare all reagents and working standards as directed in the previous sections.
2. Determine the number of microwell strips required to test the desired number of samples plus appropriate number of wells needed for running blanks and standards. Remove extra microwell strips from holder and store in foil bag with the desiccant provided at 2-8° C sealed tightly.
3. Add 100µL of Standard, control, or sample, per well. Cover with the adhesive strip provided. Incubate for 1.5 hours at 37° C.
4. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with Wash Buffer (350µL) using a squirt bottle, manifold dispenser or auto-washer. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
5. Add 100 µL of the working solution of Biotin-Conjugate to each well. Cover with a new adhesive strip and incubate 1 hour at 37° C.
6. Repeat the aspiration/wash as in step 4.

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

### AVIVA SYSTEMS BIOLOGY

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com

7. Add 100  $\mu$ L of the working solution of Streptavidin-HRP to each well. Cover with a new adhesive strip and incubate for 30 minutes at 37° C. Avoid placing the plate in direct light.
8. Repeat the aspiration/wash as in step 4.
9. Add 100  $\mu$ L of Substrate Solution to each well. Incubate for 10-20 minutes at 37° C. Avoid placing the plate in direct light.
10. Add 100  $\mu$ L of Stop Solution to each well. Gently tap the plate to ensure thorough mixing.
11. Determine the optical density of each well immediately, using a microplate reader set to 450 nm.(optionally 630nm as the reference wave length;610-650nm is acceptable)

### ASSAY PROCEDURE SUMMARY

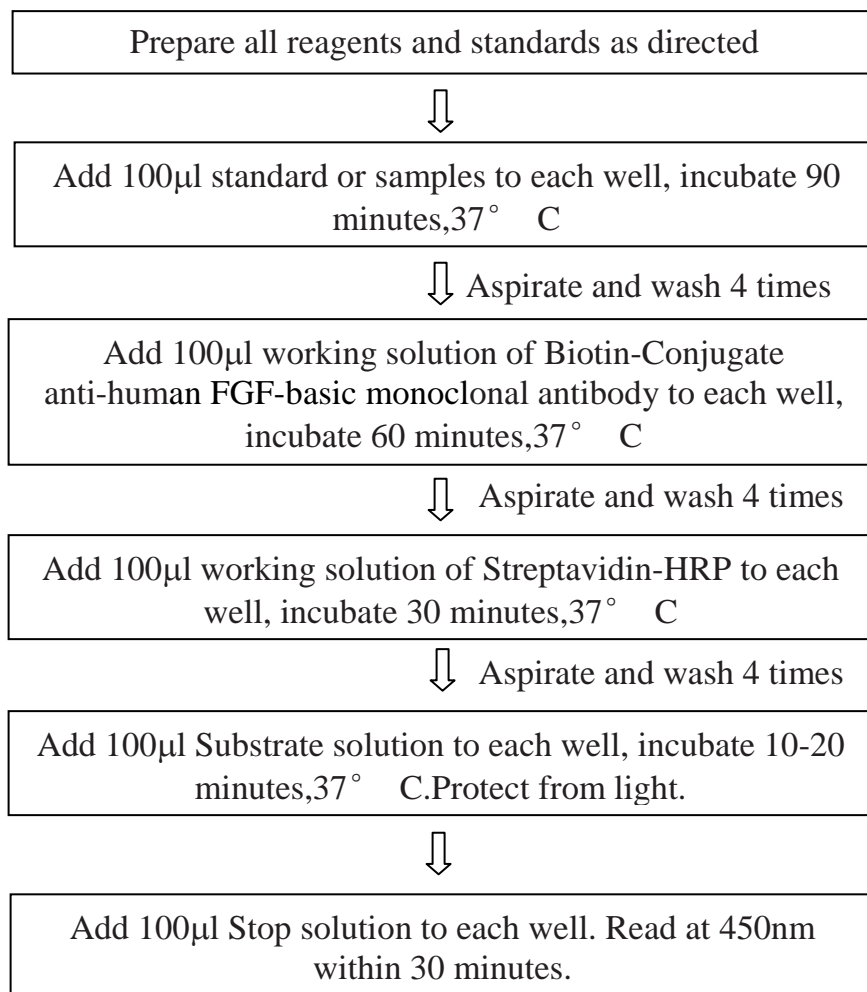


Figure 3: Assay procedure summary

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

#### AVIVA SYSTEMS BIOLOGY

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com



## TECHNICAL HINTS

1. When mixing or reconstituting protein solutions, always avoid foaming.
2. To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.
3. To ensure accurate results, proper adhesion of plate sealers during incubation steps is necessary.
4. Substrate Solution should remain colorless until added to the plate. Stop Solution should be added to the plate in the same order as the Substrate Solution. Keep Substrate Solution protected from light. Substrate Solution should change from colorless to gradations of blue.
5. A standard curve should be generated for each set of samples assayed. According to the content of tested factors in the sample, appropriate diluted or concentrated samples, it is best to do pre-experiment.

## CALCULATION OF RESULTS

1. Average the duplicate readings for each standard, control, and sample and subtract the average zero standard optical density.
2. Create a standard curve by reducing the data using computer software capable of generating a four parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph.
3. The data may be linearized by plotting the log of the FGF-basic concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.
4. This standard curve is provided for demonstration only. A standard curve should be generated for each set of samples assayed.

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

### **AVIVA SYSTEMS BIOLOGY**

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com

Table 2: Typical data using the FGF-basic ELISA (Measuring wavelength: 450nm, Reference wavelength: 630nm)

Standard (pg/ml)	OD.	OD.	Average	Corrected
0	0.052	0.049	0.051	---
7.8	0.078	0.073	0.076	0.072
15.625	0.083	0.085	0.084	0.087
31.25	0.149	0.145	0.147	0.130
62.5	0.247	0.250	0.249	0.249
125	0.548	0.542	0.545	0.555
250	1.194	1.189	1.192	1.187
500	2.067	2.059	2.063	2.064

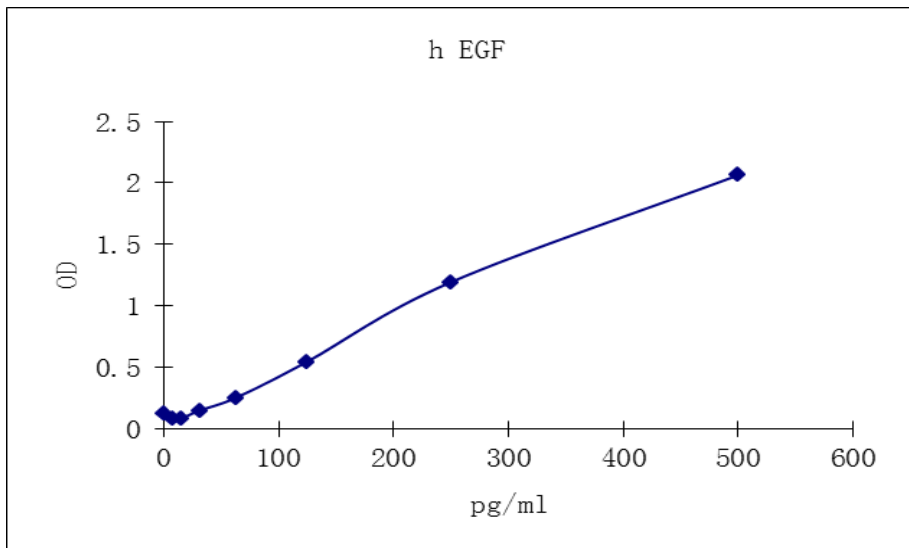


Figure 4: Representative standard curve for FGF-basic ELISA. FGF-basic was diluted in serial two-fold steps in Sample Diluent.

**Do not use this standard curve to derive test results. A standard curve must be run for each group of microwell strips assayed.**

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

**AVIVA SYSTEMS BIOLOGY**

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
 www.avivasysbio.com | Email: info@avivasysbio.com

## SENSITIVITY, SPECIFICITY AND REPEATABILITY

1. **REPEATABILITY:** The coefficient of variation of both intra-assay and inter-assay were less than 10%.
2. **SENSITIVITY:** The minimum detectable dose was 4pg/mL.
3. **SPECIFICITY:** This assay recognizes both natural and recombinant human FGF-basic. The factors listed below were prepared at 50ng/ml in Standard /sample Diluent and assayed for cross-reactivity and no significant cross-reactivity or interference was observed.

Table 3: Factors assayed for cross-reactivity

Recombinant human	Recombinant mouse	Recombinant porcine
LIF	IL-1 $\alpha$	PDGF
EGF	EGF	TGF- $\beta$ 1
TGF- $\beta$ 1	GM-CSF	
TNF- $\alpha$	TNF- $\alpha$	
TNF- $\beta$		

## REFERENCES

1. Mohammadi, M. et al. (2005) Cytokine Growth Factor Rev. 16:107.
2. Presta, M. et al. (2005) Cytokine Growth Factor Rev. 16:159.
3. Reuss, B. et al. (2003) Cell Tissue Res. 313:139.
4. Su, N. et al. (2008) Front. Biosci. 13:2842.
5. Grose, R. and C. Dickson (2005) Cytokine Growth Factor Rev. 16:179.
6. Abraham, J.A. et al. (1986) EMBO J. 5:2523.
7. Kurokawa, T. et al. (1987) FEBS Lett. 213:189.
8. Claus, P. et al. (2003) J. Biol. Chem. 278:479.
9. Quarto, N. et al. (2005) Gene 356:49.
10. Kardami, E. et al. (2004) Cardiovasc. Res. 63:458.
11. Dono, R. et al. (1998) EMBO J. 17:4213.
12. Rosenblatt-Velin, N. et al. (2005) J. Clin. Invest. 115:1724.
13. Pellieux, C. et al. (2001) J. Clin. Invest. 108:1843.
14. Montero, A. et al. (2000) J. Clin. Invest. 105:1085.
15. Miller, D. et al. (2000) Mol. Cell. Biol. 20:2260.
16. Coffin, J.D. et al. (1995) Mol. Biol. Cell 6:1861.
17. Sobue, T. et al. (2005) J. Cell. Biochem. 95:83.

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

### AVIVA SYSTEMS BIOLOGY

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com

## RELATED PRODUCTS

Table 3: Related products

Product Name	Catalog Number	Size
human EGF ELISA kit	OKAA00001	48T/96T
human Fas ELISA Kit	OKAA00002	48T/96T
human G-CSF ELISA kit	OKAA00003	48T/96T
human GDF-15 ELISA kit	OKAA00004	48T/96T
human GM-CSF ELISA kit	OKAA00005	48T/96T
human IFN-r ELISA kit	OKAA00006	48T/96T
human IL-1a ELISA kit	OKAA00007	48T/96T
human IL-2sRa ELISA kit	OKAA00008	48T/96T
human IL-3 ELISA kit	OKAA00009	48T/96T
human IL-4 ELISA kit	OKAA00010	48T/96T
human IL-5 ELISA kit	OKAA00011	48T/96T
human IL-6 ELISA kit	OKAA00012	48T/96T
human IL-9 ELISA kit	OKAA00013	48T/96T
human IL-10 ELISA kit	OKAA00014	48T/96T
human IL-12p40 ELISA kit	OKAA00015	48T/96T
human IL-12p70 ELISA kit	OKAA00016	48T/96T
human IL-15 ELISA kit	OKAA00017	48T/96T
human IL-17 ELISA kit	OKAA00018	48T/96T
human IL-21 ELISA kit	OKAA00019	48T/96T
human IL-22 ELISA kit	OKAA00020	48T/96T
human IL-32a ELISA kit	OKAA00021	48T/96T
human Leptin ELISA kit	OKAA00022	48T/96T
human MCP-1 ELISA kit	OKAA00023	48T/96T
human MMP-9 ELISA kit	OKAA00024	48T/96T
human sICAM-1 ELISA kit	OKAA00025	48T/96T
human TGF-b1 ELISA kit	OKAA00026	48T/96T
human TNF-a ELISA kit	OKAA00027	48T/96T
human TSLP ELISA kit	OKAA00028	48T/96T
human VEGF ELISA kit	OKAA00029	48T/96T
human FGF-Basic ELISA kit	OKAA00030	48T/96T
Human IL-2 ELISA kit	OKAA00031	48T/96T
Human IL-8 ELISA kit	OKAA00032	48T/96T

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURE.

---

### AVIVA SYSTEMS BIOLOGY

5754 Pacific Center Blvd., Suite 201 San Diego, CA 92121 USA | Tel: 858-552-6979  
www.avivasysbio.com | Email: info@avivasysbio.com