



## CERTIFICATE OF ANALYSIS

**Product:** Human ELN ELISA Kit

**Catalog No:** OKEH00955

**Lot No:** KF1057

**Expiration Date:** 2022.03

**Performance Characteristics:**

Intra-Assay CV	< 5.9%	Passed
Inter-Assay CV	< 7.7%	Passed
Limit of Detection (LOD)		< 0.19 ng/mL
Assay Range		0.625 – 40 ng/mL

**Standard Dilution:**


Prepare the standards immediately before use. For each experiment, add 2 mL of Sample Diluent to the 160 ng Lyophilized ELN Standard. Mix gently until dissolved. Leave the vial at ambient temperature for 15 minutes.

Prepare a 40 ng/mL Standard by adding 500 µL of 80 ng/mL Standard to 500 µL of Sample Diluent in Tube #1. Mix gently and thoroughly.

Standard Number (Tube)	Standard to Dilute	Volume Standard to Dilute (µL)	Volume Sample Diluent (µL)	Total Volume (µL)	Final Concentration (ng/mL)
Standard	160 ng/mL ELN Standard	NA	2,000	2,000	80 ng/mL
1	80 ng/mL	500	500	1,000	40 ng/mL
2	40 ng/mL	300	300	600	20 ng/mL
3	20 ng/mL	300	300	600	10 ng/mL
4	10 ng/mL	300	300	600	5.0 ng/mL
5	5.0 ng/mL	300	300	600	2.5 ng/mL
6	2.5 ng/mL	300	300	600	1.25 ng/mL
7	1.25 ng/mL	300	300	600	0.625 ng/mL
8	N/A	0	300	300	0.0 (Blank)

Sample Standard Curve and Calculations ONLY. Do not use below report for result calculations. A standard curve should be generated each time the test is performed

### Standard Curve Graph

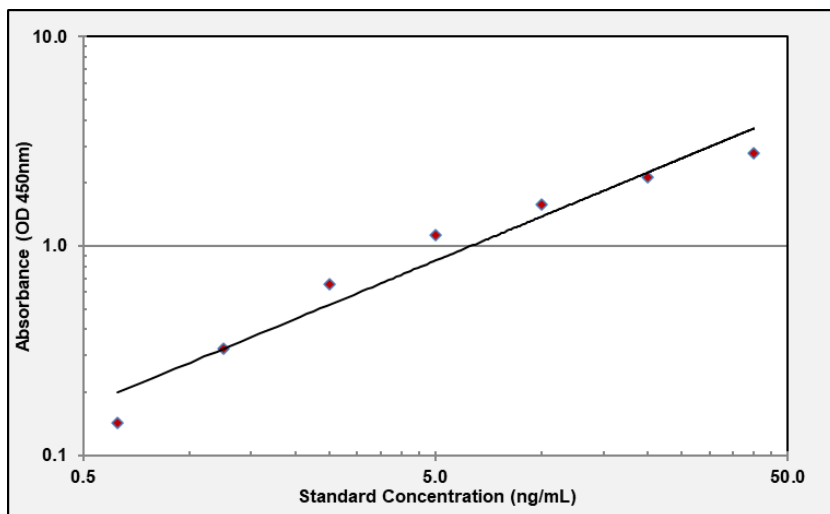

Standard ng/mL	Absorbance (OD 450nm)
40	2.790
20	2.131
10	1.587
5.0	1.133
2.5	0.654
1.25	0.323
0.625	0.143