

## CERTIFICATE OF ANALYSIS

**Product:** CAMK2A ELISA Kit (Mouse)  
**Sku:** OKEH06875  
**Lot:** KH0746  
**Expiration Date:** 2024.05

### Performance Characteristics:

|                          |         |                 |
|--------------------------|---------|-----------------|
| Intra-Assay CV           | <= 7.5% | Passed          |
| Inter-Assay CV           | <= 9.6% | Passed          |
| Limit of Detection (LOD) |         | <= 0.39 ng/mL   |
| Assay Range              |         | 0.78 - 50 ng/mL |


### Standard Preparation:

Prepare the standards immediately before use. For each experiment, add 2 mL of Sample Diluent to the 100 ng Lyophilized CAMK2A standard. Mix gently until dissolved. Leave the vial at ambient temperature for 15 minutes.

Prepare a set of diluted standards as indicated in the chart below:

| Standard Number (Tube) | Standard To Dilute           | Volume Standard To Dilute (uL) | Volume Sample Diluent Buffer (uL) | Total Volume (uL) | Final Concentration (ng/mL) |
|------------------------|------------------------------|--------------------------------|-----------------------------------|-------------------|-----------------------------|
| 1                      | Reconstitute CAMK2A Standard | N/A                            | N/A                               | 2,000             | 50                          |
| 2                      | 50                           | 300                            | 300                               | 600               | 25                          |

| Standard Number (Tube) | Standard To Dilute | Volume Standard To Dilute (uL) | Volume Sample Diluent Buffer (uL) | Total Volume (uL) | Final Concentration (ng/mL) |
|------------------------|--------------------|--------------------------------|-----------------------------------|-------------------|-----------------------------|
| 3                      | 25                 | 300                            | 300                               | 600               | 12.5                        |
| 4                      | 12.5               | 300                            | 300                               | 600               | 6.25                        |
| 5                      | 6.25               | 300                            | 300                               | 600               | 3.12                        |
| 6                      | 3.12               | 300                            | 300                               | 600               | 1.56                        |
| 7                      | 1.56               | 300                            | 300                               | 600               | 0.78                        |
| 8                      | N/A                | 0                              | 300                               | 300               | 0.0 (Blank)                 |

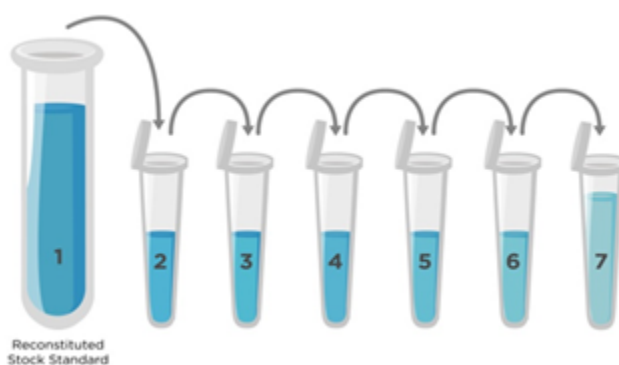

### Typical Expected Data

Standard Curve and Calculations ONLY. Do not use below report for result calculations. A standard curve should be generated each time the test is performed.

| Standard Number | Concentration (ng/mL) | Background Adjusted OD Value |
|-----------------|-----------------------|------------------------------|
| 1               | 50                    | 2.802                        |
| 2               | 25                    | 1.652                        |
| 3               | 12.5                  | 0.9                          |
| 4               | 6.25                  | 0.5                          |
| 5               | 3.12                  | 0.255                        |
| 6               | 1.56                  | 0.117                        |

| Standard Number | Concentration (ng/mL) | Background Adjusted OD Value |
|-----------------|-----------------------|------------------------------|
| 7               | 0.78                  | 0.049                        |

Standard Curve Graph

